




Spectral Irradiance

Spectral Power Distribution (SPD) for QUV/uvc testers with UVC-254 Lamps

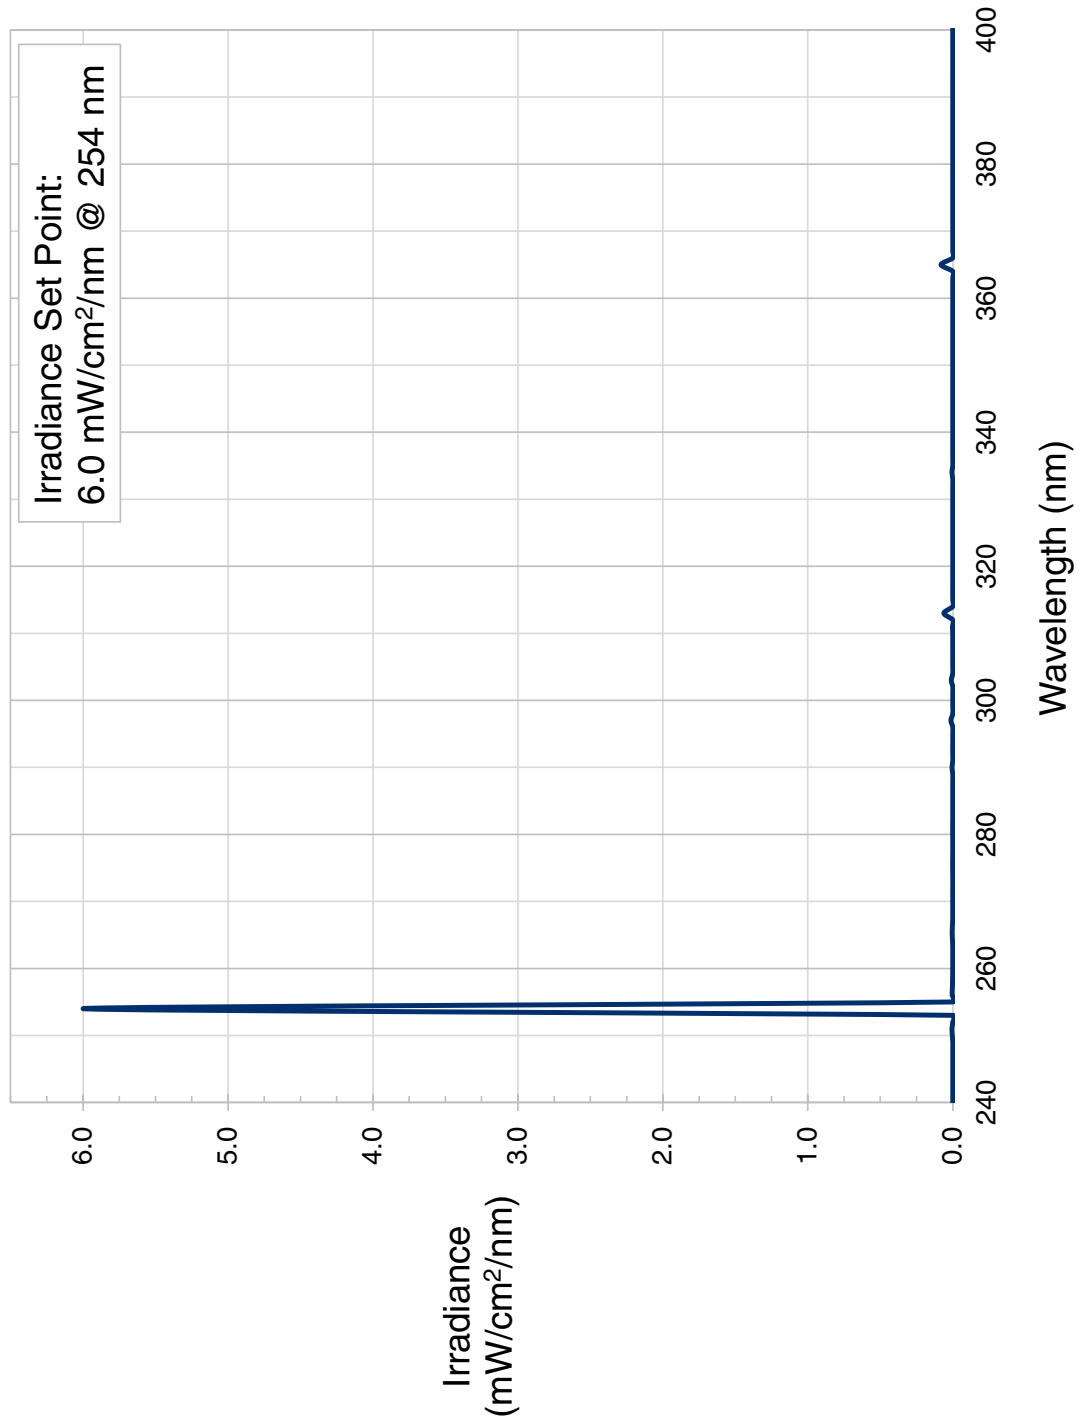

NOTES

- Irradiance from UVC-254 lamps is concentrated around the 254 nm line – peak width shown may represent instrumental limitation.
- No irradiance at the 185 nm line is emitted from the lamp (region not shown on graph).
- Irradiance peak height shown is representative. See [LU-0819 QUV Specifications](#) for irradiance capabilities.



For sales, technical, or repair support, please visit:

[Q-Lab.com/UVLamps](https://www.q-lab.com/UVLamps)

Westlake, Ohio USA • Homestead, Florida USA • Buckeye, Arizona USA
Bolton, England • Saarbrücken, Germany • Shanghai, China